


Smilekey How-to-Quick Guide

Smilekey Tip is designed to be positioned 10mm from the center of coping.

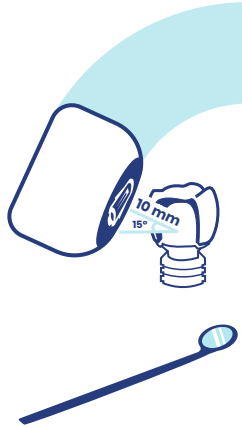


We recommend to move tip from soft tissue to occlusion during activation. Repeat activation on opposite side for another 4 seconds if necessary.

8 seconds (2 back-to-back) for Zirconia, eMax and porcelain prosthesis.

Metal objects, such as retractors, mirrors, etc., should not be near during Smilekey activation.

Smileloc icon indicates the activation side.

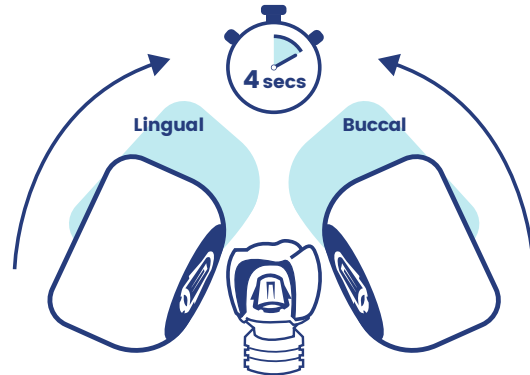

4 seconds for Acrylic, PMMA, Resin prosthesis.


Angle tip toward the center of coping. Avoid pointing at implant.



Please refer to IFU0004 for Full Product Information

Smilekey How-to-Quick Guide

▲ Smileloc icon indicates the activation side.

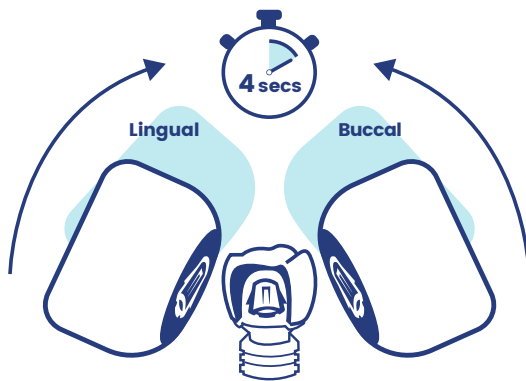


▲ 4 seconds for Acrylic, PMMA, Resin prosthesis.

▲ 8 seconds (2 back-to-back) for Zirconia, eMax and porcelain prosthesis.

▲ Angle tip toward the center of coping. Avoid pointing at implant.

▲ We recommend to move tip from soft tissue to occlusion during activation. Repeat activation on opposite side for another 4 seconds if necessary.

▲ Metal objects, such as retractors, mirrors, etc., should not be near during Smilekey activation.



▲ Smilekey Tip is designed to be positioned 10mm from the center of coping.



Smileloc
BY RODO



Please refer to IFU0004 for Full Product Information